



QuickTOCNPO

TN_b/TP-ANALYSIS

TOC, TN_b, TP and COD – combined in one analyser.
Cost efficient monitoring of WWTP's effluent.

Fast. Precise. Reliable.



FOUR PARAMETERS. ONE ANALYSER.

The sumparameters TOC, COD, TNb and TP are the most important ones with in the field of waste water. Their combination in one analyser is worth it.



— An over-fertilization (eutrophication) of water with nitrogen and phosphorus leads to an ecological imbalance that causes harmful vegetation: The QuickTOC_{NPO} is optimally suitable for the monitoring of waste water effluent in order to avoid the discharge of contaminated water into rivers and lakes.

The effluent control of industrial and municipal waste water treatment plants is of special importance – either in ecological and economic point of view. By continuous measurements the treatment performance maybe monitored. The effluent finally is discharged into river water and/or lakes which can be better protected.

— TOC, TNb, TP and COD. Monitoring of regulated waste water parameters.

The monitoring of the effluent of waste water treatment plants (WWTP) is regulated by local authorities. The effluent levels of TOC, TNb, TP and COD into public waters vary depending on the country and/or municipality. Each may have an own defined waste water regulation. However, the aim of such legal frameworks for water management is to protect water as a meaningful part of ecosystems, as natural basis of life for humankind as well as for flora and fauna.

Generally, four different analysers are needed in order to monitor the four sum parameters. With the help of combined measurement systems, a more cost efficient monitoring can be established.

— What TOC means and how it is measured.

A whole variety of organic matter can be present in water, which cannot be determined individually. At least not without considerable analytical effort and with in a short time. This is why the so-called sum parameter TOC (total organic carbon) is used. It measures a samples organic loads and is thus an important indicator for water quality.

The TOC content is best detected by using the thermal combustion at 1,200°C. It ensures that all organic carbon bonds are oxidised, producing CO₂ which can then be detected, quantitatively measured and calculated and reported as TOC.

At 1,200°C,
water samples
are completely
and precisely
analysed.

What TNb means and how it is measured.

The TNb (total nitrogen bound) shows the pollution of water caused by nitrogen compounds. Nitrogen may be present as ammonia, ammonium salts, nitrites, nitrates and organic nitrogen compounds. In contrast to single measurements of the above mentioned components, the TNb determination contains all these substances in a single analysis process.

The accumulation of nitrogen compounds in water leads to an unwanted increase of nutrients (eutrophication). Such an exceeding leads to a harmful plant growth. Certain plants such as algae for instance spread rampantly and disturb the eco-logical balance massively. Hence, the TNb is an important parameter for the assessment of waste water.

The most common method for the determination of TNb is the combustion of nitrogen oxides. Subsequently, by use of an electro chemical cell (EC cell) or a chemiluminescence detector (CLD) the TNb content will be detected.

What TP means and how it is measured.

The TP (total phosphorus) is a sum parameter that measures the organic and inorganic phosphorus compounds in water. Phosphorus is an essential nutrient for humans as well as flora and fauna. However, the substance – depending on its concentration – may cause serious damage. Generally, phosphorus is a naturally limited substance. Its sources are for instance soil and stones, waste water, animal waste and decay of organic substances.

Increased phosphorus concentration affect the quality of water and lead to algal blooms, an increased growth of plants and a

decreased concentration of dissolved oxygen due to the additional vegetation. Hence, the TP is an important parameter when it comes to direct discharge of waste water in to public water bodies.

The TP content is determined by ortho phosphate (PO₄³⁻). During the wet chemical oxidation there is a reducing agent added to the sample. Subsequently, the sample mixture is led through an UV reactor. The ultra violet light oxidises dissolved and bound phosphorus compounds to phosphate (PO₄³⁻). On leaving the reactor the TP content is quantitatively determined by use of molybdenum blue.

What COD means and how it is measured.

The COD (chemical oxygen demand) stands for the amount of oxygen that is needed for the oxidation of all organic and inorganic ingredients contained in the water sample. It is also considered when it comes to planning and controlling of waste water treatment plants as it shows the treatment efficiency of a WWTP. Furthermore, it is basis for the calculation of discharge fees. Hence, it is an important parameter.

The COD is determined by use of the oxidizability of the organic carbons.

AT A GLANCE

- The parameters TOC, Tnb, TP & COD are important for discharge control.
- The combination of these parameters minimizes costs of investment, maintenance and service.
- At 1,200°C no catalyst is necessary.
- Complete combustion of organic and inorganic nitrogen compounds.
- LAR is the only supplier offering an analyser that combines Tnb and TP with TOC and COD in one unit

THE ANALYSER.

A hot oven: Where temperature makes the difference.

Warm, warmer, hot.

Tracking pollution at 1,200°C.

The catalyst-free ceramic oven is the centre piece of the QuickTOC_{NP0}. At 1,200°C, it reliably dissolves all carbon bonds and thus enables a complete analysis of samples. Despite the high temperatures used, absolute safety is guaranteed in all settings. For this end, the QuickTOC_{NP0} can be delivered with a number of different housings, depending on the intended location. That way the analyser itself can be safely at high corrosive places as well as in Ex-Zones.

All in one.

The accurate determination of 4 parameters.

Due to the fact that the thermal oxidation is complete as well as the close relation between TOC and COD it is very easy to correlate both parameters.

In addition, all parameters are determined in accordance to international standards.

The total phosphorus is determined by the photo metric molybdenum blue method. First, the sample is being mixed with an oxidising agent. Subsequently, the mixture is led in to the reactor where ultra violet light (UV) activates the sample's oxidation. Finally, by adding the molybdenum blue it becomes visible how much TP is in the sample.

The building blocks principle for a tailor made measurement instrument.

The modular system offers high flexibility. When your application demand sit, you can measure the parameters in combination or for example TP only. Furthermore, you can decide whether to build in additional detectors to determine the TNb and COD parameters alongside measuring the TOC.

Ultra quick measurements and maintenance.

The TNb measurement takes place in less than 3 minutes - as prompt at the TOC value. Thereby, even short measurement value peaks can also be reliably shown. The maintenance service is also fast: Less than half an hour per week. The analyser's availability is over 98%. More over, all areas of the analyser have been designed for easy maintenance: From the generously measured and blockage-free tubes to the catalyst-free high temperature oven.

Sample taking. Matrix-matched.

Depending on the composition of the sample the sample taking may differ. Under normal circumstances the outlet/effluent of a sewage plant is free of particles—or at least there are only a few. In this case a centrifugal separator is sufficient for the sample extraction. However, is the sample characterised by a high particle density, the sample should be taken by the filterless, patented Flow Sampler.

With the QuickTOC_{NP0} the analytical area is isolated from the electronics.

All areas are easily accessible.



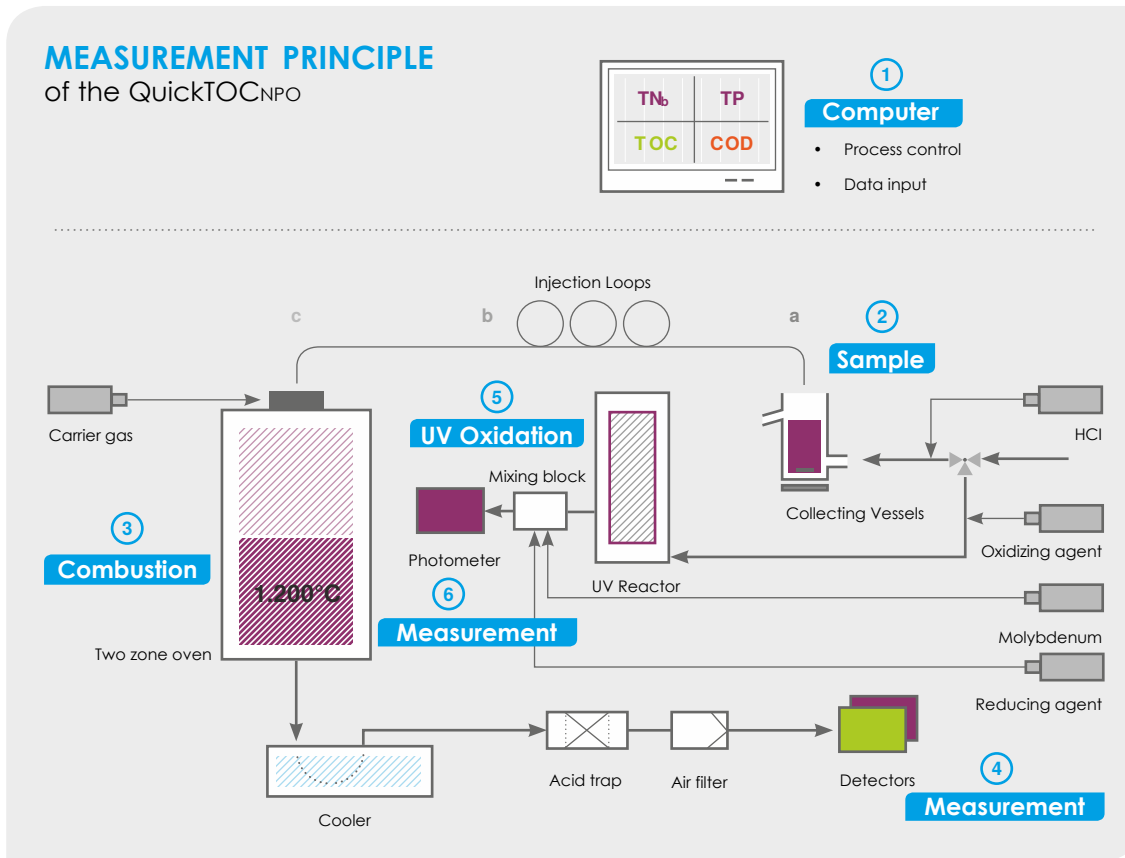


Fig.2

- 1) Process Control, display of measurement results, interfaces to the periphery.
- 2) Sample transportation via injection loop
 - a) Extraction of sample from sample stream
 - b) Definition of sample volume
 - c) Injection through lock valve
- 3) Combustion, oxidation to CO₂ and NO
- 4) Measurement of CO₂ and NO concentration
- 5) UV-Oxidation to PO₄³⁻
- 6) Measurement of TP concentration

THE PRINCIPLE.

The innovative complete solution for effluent monitoring at WWTPs.

The closed injection system . Exact sample dosing.

With in the analyser at first the sample is kept homogenised in the sample vessel. Then an exactly dosed sample volume is being sucked through a closed tubing system and injected into the reactor passing the special lock valve.

Inert materials and a pump that is installed downstream make sure that no memory effects of previous measurements occur. Additionally, the special lock valve ensures that the oven is 100% closed against ambient air so that no contamination can happen.

Inside of the ceramic oven: We like it hot.

And it is that hot, that - without catalysts - the sample's content of Nitrogen and Carbon is completely converted into NO and CO₂. It is oxidised by use of a carrier gas that is supplied by filtered pressurised air. Optionally, the QuickTOC_{NPO} can prepare the gas itself requiring no extra external gas supply at all. Through the high temperature, the salts present can easily be discharged. They move through the oven in fluid form and are carried out of the oven by the condensate. Finally, they are deposited in a retaining device, from which they can easily and quickly be removed. That way, no salt deposits can accumulate in the oven.

The NO detection. It is your choice.

First the gas that is produced by the combustion condenses in the cooler. The remaining combustion gas is purified by a filter before its NO concentration is determined by an electrochemical cell (ECD) or, alternatively, a chemiluminescence detector (CLD).

The CO2 detection.

Reliable and simple.

Following the TNb determination the gas mixture is transported using the carrier gas to a CO2 detector which quantifies the carbon dioxide and detects the TOC content.

The molybdenum blue method.


A photometric analysis.

In order to measure the total phosphorus the sample is mixed with the oxidising agent persulfate.

Subsequently, the sample mixture is led into the UV reactor, where the sample together with the persulfate is oxidised to orthophosphate ((PO₄)). The produced PO₄-reacts with ammonium molybdate to a molybdenum phosphoric acid which forms molybdenum blue with added reducing agents. This molybdenum blue is measured by a photometer and displayed as TP.

The molybdenum blue method is more accurate than other methods and allows the detection of low TP concentrations.

Fig.3

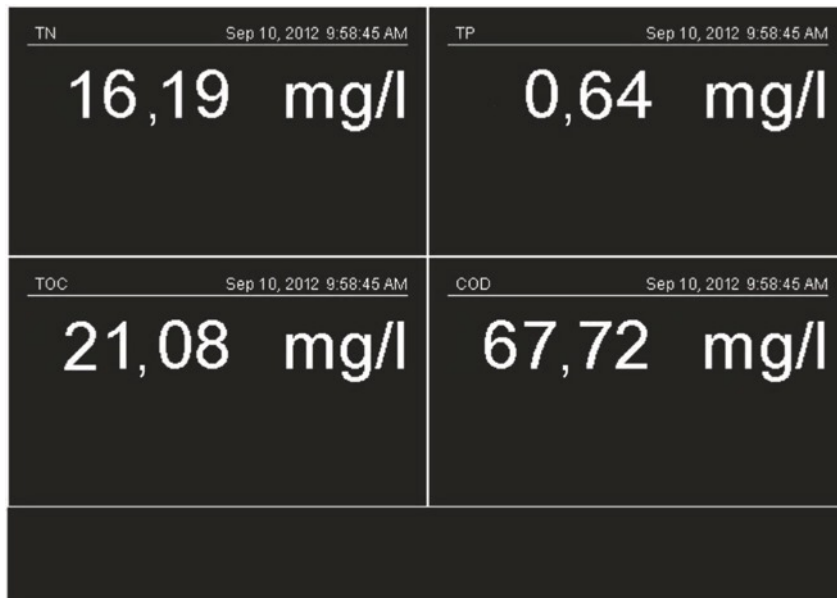

The figure gives an example of the QuickTOC_{NPO}'s display showing all four parameters while monitoring the effluent stream of a waste water treatment plant.

You can individually decide how the parameter values should be displayed.

ALL cLeAR?

LAR Process Analysers AG: Water is our Element.
We do every thing for its protection.

We are the leading provider for water analysis instruments for industrial and communal waste water technology, process monitoring, as well as for pure water analysis. Further products in the areas of industrial process and environmental technology complete our product range.

LAR offers application specific analysers developed by our research and development team. Maintenance is carried out globally by our own technicians or by our local qualified service partners. Technical support per telephone or e-mail is available at all times.

TOC-ANALYSIS

From complex industry waste water to pharmaceutical pure water, our TOC analysers determine parameters quickly and precisely.

COD-ANALYSIS

With our analysers the chemical oxygen demand is cleanly and safely determined online, without using chemicals.

BOD/TOXICITY

We detect the BOD with the plant's own biomass and determine the toxicity with highly sensitive bacteria. Fast and reliably.

TNb/TP-ANALYSIS

TNb and TP are important parameters for waste water treatment. We are the only ones who offer them in combination with TOC and COD in one system.

FURTHER PRODUCTS

LAR offers a specific solution for nearly all applications. With our protective housings, you are on the safer side. Find out more: www.lar.com

QuickTOC_{NPO} AN OVERVIEW

The online monitoring of TOC, TN_b, TP and COD - in one analyser.

The Quick TOC_{NPO} monitors continually the effluent streams of waste water treatment plants in order to determine the most important parameters fast. The sum parameters may be selected and adjusted in accordance to the requirements of the application.

QTNPO-1 E 0214

TECHNICAL DATA

Measurement Technique and Sample Preparation

Measurement Ranges	TOC: 0.1 – 50 mg/l, max. 200 mg/l TN _b : 0.1 – 30 mg/l, max. 200 mg/l TP: 0.01 – 3 mg/l, max. 30 mg/l COD: 1 – 150 mg/l, max. 600 mg/l
--------------------	--

Response Time	TOC/ COD: 2 – 3 minutes TN _b : 1 – 3 minutes TP: 10 – 15 minutes
---------------	---

Sample Preparation	Centrifugal separator F lowSampler
--------------------	---------------------------------------

Dimensions and Weight

Housing	Steel IP 54, powdercoated
Options	Stainless steel, IP 65, ATEX Zone 1a and 2 for T3 and T4 classes (national standards on request)
Dimensions	670 x 1,070 x 550 mm (W x H x D)
Weight	115 kg (Standard)

Electric and Hydraulic Specifications

Inflow and Outflow	Tube 3.2 mm ID, Tube 12 mm ID
Auxiliary Energy	230/115 V~, 50/60 Hz
Analogue Output	0/4– 20 mA
Serial Interface	RS 232
Safety	10 A intern, 16 A extern
Remote Control	option: via TCP/IP protocol (Internet)

Equipment Devices and Data Output

LC-Display, 230 x 100 mm (W x H), back lit
Autostart function
Self explanatory software
Standard data interfaces to office PC (USB)



Fast and precise –
the QuickTOC_{NPO}
is reliable!



ADVANTAGES & FEATURES

- ✓ exact determination of four parameters: TOC, TN_b, TP and COD
- ✓ selectable parameter combination
- ✓ highest combustion temperature available (1,200°C)
- ✓ detection of TN_b by cost effective ECD (CLD optional)
- ✓ molybdenum blue method for the determination of TP
- ✓ no filtration of sample necessary
- ✓ analyser availability minim. 98%
- ✓ maintenance and service max. 30 min per week
- ✓ exceptionally low maintenance and operational costs

LAR Process Analysers AG

Neukoellnische Allee 134
D-12057 Berlin
www.lar.com

Phone +49 30 278 958-43Fa
x +49 30 278 958-703
E-Mail export@lar.com



TÜV certified company

TN_b/TP/TOC/COD-ANALYSIS

QuickTOC_{NPO}

AREAS OF APPLICATION

ENVIRONMENT / MUNICIPAL FACILITIES / INDUSTRY

INDUSTRIES

**ENVIRONMENTAL MONITORING / WASTE WATER TREATMENT /
WASTE PROCESSING / PHARMACEUTICAL / LABORATORY / PETRO- CHEM
ICAL / REFINERIES / CHEMICAL / COAL AND STEEL / POWER / AIRPORTS
/ AUTOMOBILE / PAPER MANUFACTURE / BREWERIES / FOOD MANUFACT
URE / DRINK MANUFACTURE/ MILK PROCESSING**

TYPES OF WATER

**GROUNDWATER / SURFACE WATER / DRINKING WATER /
WATER INFLUENT / WATER EFFLUENT / DISCHARGE CONTROL /
INDUSTRIAL WASTE WATER / DE-ICING WATER / PROCESS WATER / OIL
-IN-WATER / HIGH SALT CONCENTRATION / COOLING WATER /
PURE WATER / BOILER FEED WATER / CONDENSATE RETURN /
PHARMA HPW / PHARMA WFI**



Envitech Ltd

Unit S7
Capital Business Park
Parkway
Cardiff
CF3 2PU

Email: info@envitech.co.uk

Tel: 0044 2920 364252

Web: www.envitech.co.uk