


NANOCOLOR® Phosphat 50




Method(e):

0791
10.0 - 50.0 mg/l P


0792
30 - 150 mg/l PO₄³⁻

0793
23 - 110 mg/l P₂O₅


REF 985 079

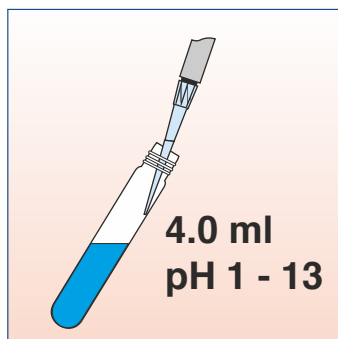


Sample

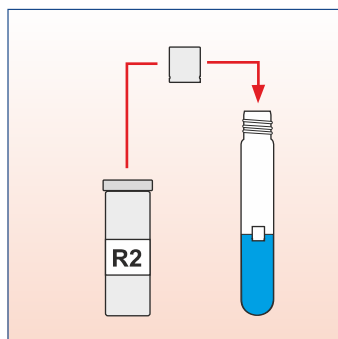


1 x **NANOFIX R2**

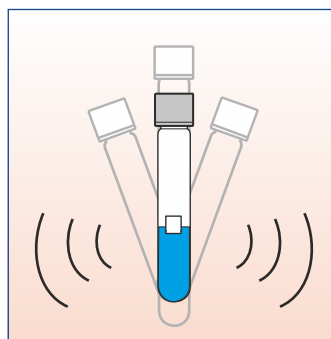


Shake

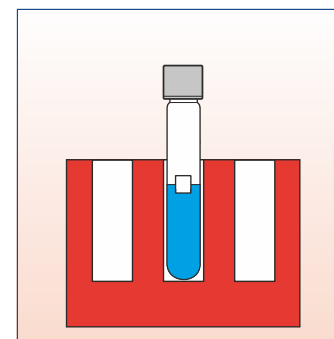


120 °C / 30 min
100 °C / 1 h

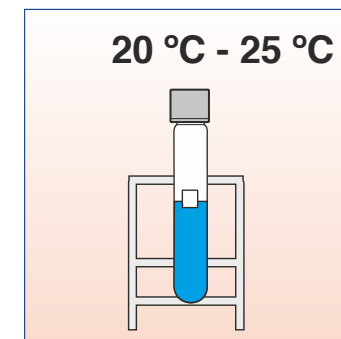


Cool

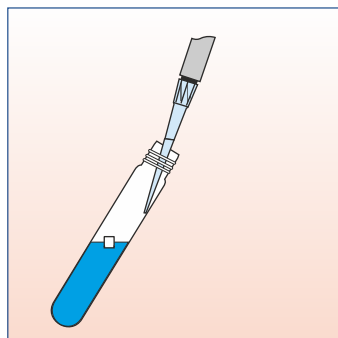


1.0 ml R3

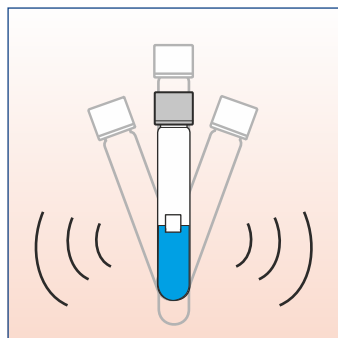

Shake

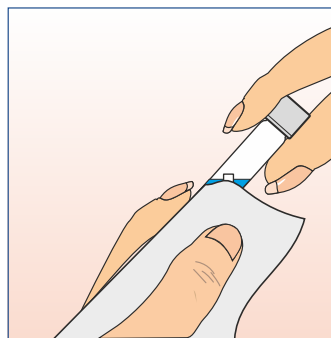


Clean

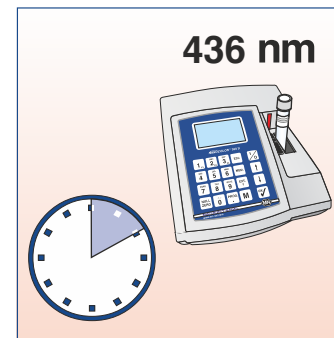

Measure

NANOCOLOR[®] ortho-Phosphat 50 / Phosphate / Fosfato




Method(e):

0794
10.0 - 50.0 mg/l PO₄-P


0795
30 - 150 mg/l PO₄³⁻

0796
23 - 110 mg/l P₂O₅


REF 985 079

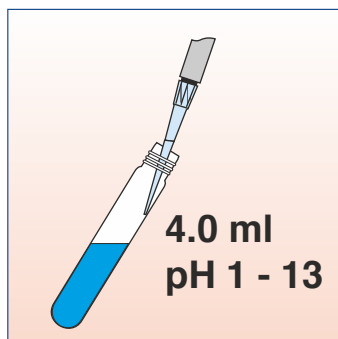


Probe / Sample
Échant. / Muestra

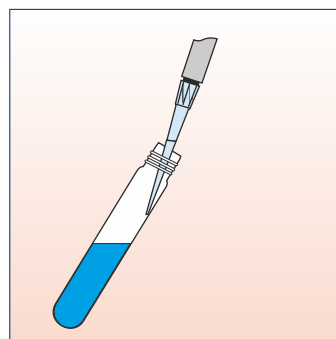


1.0 ml R3

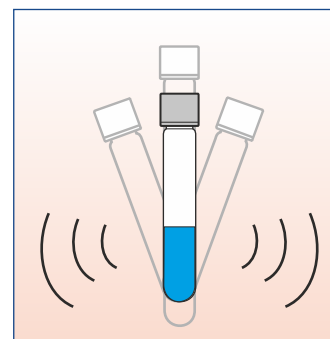


Schütteln / Shake
Agiter / Agitar

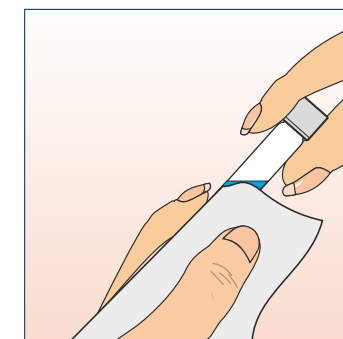

Säubern / Clean
Nettoyer / Limpiar

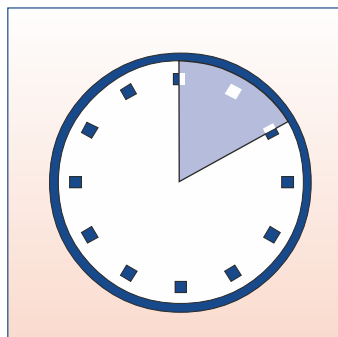

10'00 min

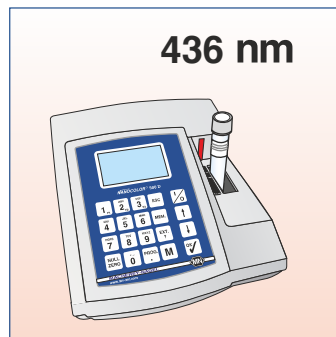

Messen / Measure
Mesurer / Medir